


HP 03458-66509 (A9 reference board)

This is a clone of the reference board in the HP 3458A 8.5-digit multimeter.

See <https://github.com/pepaslabs/hp-03458-66509-clone>

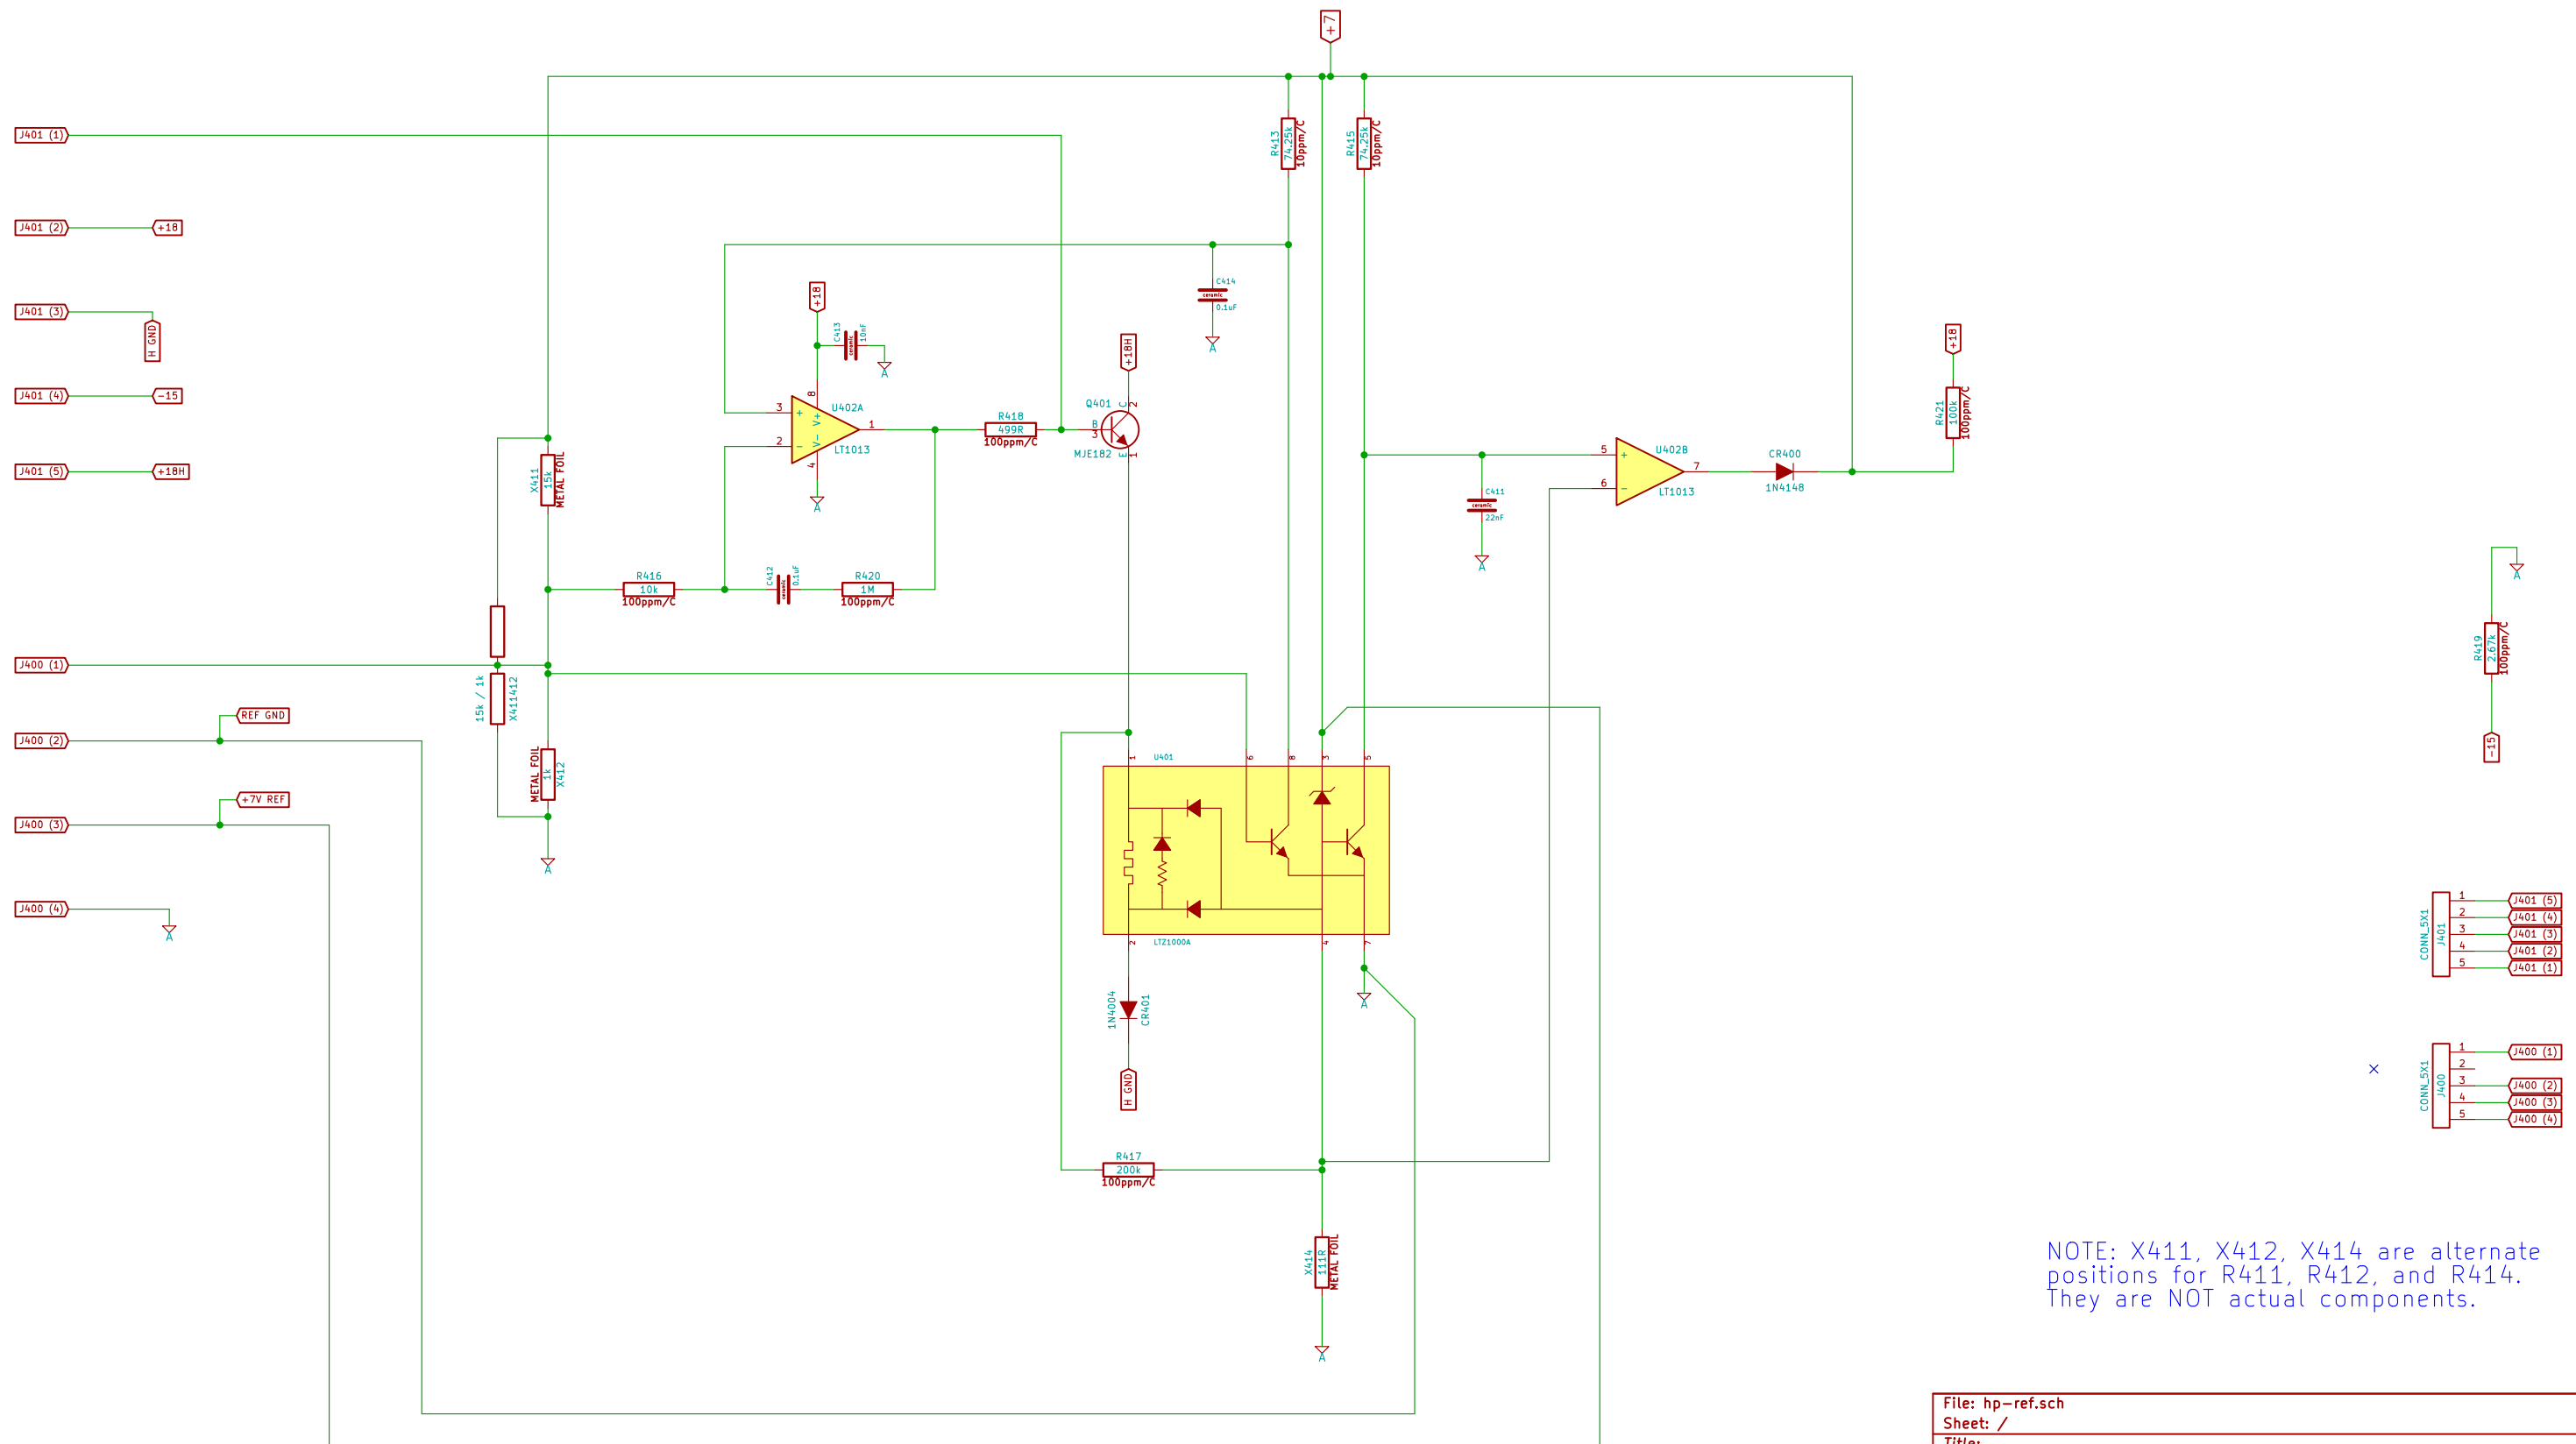

NOTE: X411, X412, X414 are alternate positions for R411, R412, and R414. They are NOT actual components.